



Porcine AMH ELISA

RUO

AL-169

INTENDED USE

The Porcine Anti-Müllerian hormone (AMH) enzyme-linked immunosorbent assay (ELISA) kit provides materials for the quantitative measurement of AMH in porcine serum and other biological fluids.

SUMMARY AND EXPLANATION

Anti-Müllerian hormone is a 140 kDa glycoprotein that is produced during normal embryogenesis by the Sertoli cells of the embryonic testis, causes the involution of the Müllerian duct, and inhibits female gonadogenesis by inducing apoptosis of target gonadal cells. It belongs to the transforming growth factor- β super family. AMH causes apoptosis of specific Anti-Müllerian inhibiting substance (MIS) receptor-bearing cells, while having no effect on cells without receptors. AMH is also expressed in granulosa cells of preantral and small antral follicles in the ovary, and AMH inhibits recruitment of primordial follicles into the pool of growing follicles, and decreases responsiveness of growing follicles to FSH.

PRINCIPLE OF THE TEST

The Porcine AMH ELISA is a quantitative three-step sandwich type immunoassay. In the first step, serially diluted Calibrators and unknown samples are added to AMH antibody coated micro titer wells and incubated. After the first incubation and washing, the wells are incubated with biotinylated AMH antibody solution. After the second incubation and washing, the wells are incubated with streptavidin horseradish peroxidase conjugate (SHRP) solution. After the third incubation and washing step, the wells are incubated with substrate solution (TMB) followed by an acidic stopping solution. In principle, the antibody-biotin conjugate binds to the solid phase antibody-antigen complex which in turn binds to the streptavidin-enzyme conjugate. The antibody-antigen-biotin conjugate-SHRP complex bound to the well is detected by enzyme-substrate reaction. The degree of enzymatic turnover of the substrate is determined by dual wavelength absorbance measurement at 450 nm as primary test filter and 630 nm as reference filter. The absorbance measured is directly proportional to the concentration of AMH in the samples and calibrators.

MATERIALS SUPPLIED

CAL-105A AMH/MIS Calibrators A / Sample Diluent

One bottle, 11 mL, labeled AMH/MIS Cal A/Sample Diluent, containing 0 ng/mL AMH in protein-based buffer and ProClin 300. Store unopened at 2-8°C until the expiration date.

CAL-169H AMH Calibrator H (Lyophilized)

One vial, labeled H, containing concentration of approximately 16 ng/mL AMH in protein-based buffer and ProClin 300. Refer to calibration card for exact concentration. Store unopened at 2 to 8°C until the expiration date. Reconstitute calibrator H with **1 mL** deionized water. Solubilize, mix well and

use after reconstitution. Aliquot and Freeze in plastic vials for multiple use. Alternatively, freeze in the same vial within 2 hours of reconstitution. Avoid repeated freeze thaws.

PLT-113 AMH Coated Microtitration strips

One strip holder, containing 12 strips and 96 microtitration wells with AMH antibody immobilized to the inside wall of each well. Store at 2-8°C until expiration date in the resealable pouch with a desiccant to protect from moisture.

ASB-116 Canine AMH Assay Buffer

One bottle, 10 mL, containing a protein-based (BSA)-buffer with a non-mercury preservative. Store at 2-8°C until expiration date.

BCR-169 AMH Biotin Conjugate Ready-To-Use (RTU)

One bottle, 12 mL, containing biotinylated anti-AMH antibody in protein-based buffer with a non-mercury preservative. Store at 2-8°C until expiration date.

SAR-169 AMH Streptavidin-Enzyme Conjugate-Ready-to-Use (RTU)

One amber bottle, 12 mL, containing Streptavidin-HRP (horseradish peroxidase) in a protein-based buffer and a non-mercury preservative. Store undiluted at 2-8°C until expiration date.

TMB-100 TMB Chromogen Solution

One bottle, 11 mL, containing a solution of tetramethylbenzidine (TMB) in buffer with hydrogen peroxide. Store at 2-8°C until expiration date.

STP-100 Stopping Solution

One bottle, 11 mL, containing 0.2 M sulfuric acid. Store at 2 to 30°C until expiration date.

WSH-100 Wash Concentrate A

One bottle, 60 mL, containing buffered saline with a nonionic detergent. Store at 2-30°C until expiration date. Dilute 25-fold with deionized water prior to use.

MATERIALS REQUIRED BUT NOT PROVIDED

1. Microtitration plate reader capable of absorbance measurement at 450 nm, 405nm and 630 nm.
2. Microplate shaker.
3. Microplate washer.
4. Semi-automated/manual precision pipette to deliver 10–250 μ L.
5. Disposable 12 x 75 mm culture tubes.
6. Vortex mixer.
7. Deionized water.

WARNINGS AND PRECAUTIONS

For Research Use Only.

The following precautions should be observed:

- Follow good laboratory practice.
- Use personal protective equipment. Wear lab coats and disposable gloves when handling immunoassay materials.
- Handle and dispose of all reagents and material in compliance with applicable regulations.

WARNING: Potential Biohazardous Material

This reagent may contain some animal and/or human source material (e.g. serum) or materials used in conjunction with human source materials. Handle all reagents and patient samples at a Biosafety Level 2, as recommended for any potentially infectious human material in the Centers for Disease Control/National Institutes of Health manual "Biosafety in Microbiological and Biomedical Laboratories," 5th Edition, 2007¹.

WARNING: Potential Chemical Hazard

Some reagents in this kit contain ProClin 300 and Sodium azide² as a preservative. ProClin 300 and Sodium azide in concentrated amounts are irritants to skin and mucous membranes.

For further information regarding hazardous substances in the kit, please refer to the MSDS, either at AnshLabs.com or by request.

SAMPLE COLLECTION AND PREPARATION

- Serum is the recommended sample type.
- Sample handling, processing, and storage requirements depend on the brand of blood collection tube that you use. Please reference the manufacturer's instructions for guidance. Each laboratory should determine the acceptability of its own blood collection tubes and serum separation products.
- Samples may be stored at 4°C if assayed within 24 hours; otherwise samples must be stored at -20°C or -80°C to avoid loss of bioactivity and contamination.
- Avoid assaying lipemic, hemolyzed or icteric samples.
- Avoid repeated freezing and thawing of samples. Thaw samples no more than 3 times.
- For shipping, place specimens in leak proof containers in biohazard specimen bags with appropriate specimen identification and test requisition information in the outside pocket of the biohazard specimen bag. Follow DOT and IATA requirements when shipping specimens³.


PROCEDURAL NOTES

- A thorough understanding of this package insert is necessary for successful use of the Porcine AMH ELISA assay. It is the laboratory's responsibility to validate the assay for their use. Accurate results will only be obtained by using precise laboratory techniques and following the package insert.
- A calibration curve must be included with each assay.
- Bring all kit reagents to room temperature before use. Thoroughly mix the reagents before use by gentle inversion. Do not mix various lots of any kit component and do not use any component beyond the expiration date.
- Use a clean disposable pipette tip for each reagent, calibrator, control or sample. Avoid microbial contamination of reagents, contamination of the substrate solutions with the HRP conjugates. The enzyme used as the label is inactivated by oxygen, and is highly sensitive to microbial contamination, sodium azide, hypochlorous acid and aromatic chlorohydrocarbons often found in laboratory water supplies. Use deionized water.

- Incomplete washing will adversely affect the outcome and assay precision. Care should be taken to add TMB into the wells to minimize potential assay drift due to variation in the TMB incubation time. Avoid exposure of the reagents to excessive heat or direct sunlight.

PREPARATION OF REAGENTS

- AMH Calibrators B-G:**
 - Tap and reconstitute AMH Calibrator H with 1 mL deionized water. Solubilize for ten minutes, mix well before use.
 - Prepare seven polystyrene tubes and label them as Cal A, Cal B, Cal C, Cal D, Cal E, Cal F and Cal G.
 - Add **500 µL** of AMH/MIS Calibrator A/Sample Diluent to each polystyrene tube labeled Cal A-G.
 - Add **500 µL** of reconstituted AMH Calibrator H (from step a) to the tube labeled Cal G. Vortex and mix the content in the tube thoroughly before the next dilution transfer.
 - Add **500 µL** of Cal G (from step d) to the tube labeled Cal F. Vortex and mix the content in the tube thoroughly before the next dilution transfer.
 - Add **500 µL** of Cal F (from step e) to the tube labeled Cal E. Vortex and mix the content in the tube thoroughly before the next dilution transfer.
 - Add **500 µL** of Cal E (from step f) to the tube labeled Cal D. Vortex and mix the content in the tube thoroughly before use.
 - Add **500 µL** of Cal D (from step g) to the tube labeled Cal C. Vortex and mix the content in the tube thoroughly before use.
 - Add **500 µL** of Cal C (from step h) to the tube labeled Cal B. Vortex and mix the content in the tube thoroughly before use.
 - Note:** If more sensitivity is desired, Cal B can be further diluted to B/2 and B/4 using Cal A.
 - **Cal. B/2:** Mix 100 µL of Cal B (from step i) with 100 µL of calibrator A.
 - **Cal. B/4:** Mix 50 µL of Cal B (from step i) with 150 µL of calibrator A.
 - The tube labeled Cal A contains **500 µL** AMH Calibrator A/Sample Diluent and has 0 AMH concentrations and should be used as Blank.
 - The Calibrators A-G for instance should read as 0.0, 0.39 ng/mL, 0.78, 1.56, 3.125, 6.25, 12.5 and 25 ng/mL. Aliquot and freeze the AMH Cal H Stock immediately for multiple uses. Avoid repeated freeze thaws. Frozen aliquots at -20°C are good for one year.
 - The AMH concentration in the AMH calibrators H is traceable to the manufacturer's working calibrators. Values assigned by other methodologies may be different. Such differences, if present, may be caused by inter-method bias.

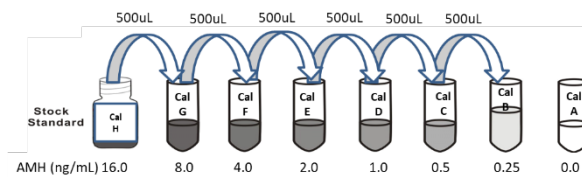

- Wash Solution:** Dilute wash concentrate 25-fold with deionized water. The wash solution is stable for one month at room temperature when stored in a tightly sealed bottle.
- Microtitration Wells:** Select the number of coated wells required for the assay. The remaining unused wells should be placed in the resealable

pouch with a desiccant. The pouch must be resealed to protect from moisture.

ASSAY PROCEDURE

Allow all specimens and reagents to reach room temperature and mix thoroughly by gentle inversion before use. Calibrators and unknowns should be assayed in duplicate.

NOTE: All serum samples reading higher than the highest calibrator should be mixed and diluted in the 0 ng/mL Calibrator A/Sample diluent prior to assay.

1. Label the microtitration strips to be used.
2. Pipette **50 µL** of the Calibrators (Cal A-G), controls and unknowns to the appropriate wells.
3. Add **50 µL** of the Canine AMH Assay Buffer to each well using a repeater pipette.
4. Incubate the plate, shaking at a fast speed (**600-800 rpm**) on an orbital microplate shaker, for **120 minutes** at room temperature.
5. Aspirate and wash each strip **5 times** with Wash Solution using an automatic microplate washer.
6. Add **100 µL** of the Antibody-Biotin Conjugate RTU to each well using a repeater pipette.
7. Incubate the plate, shaking at a fast speed (**600-800 rpm**) on an orbital microplate shaker, for **60 minutes** at room temperature.
8. Aspirate and wash each strip **5 times** with the Wash Solution using an automatic microplate washer.
9. Add **100 µL** of the Streptavidin-Enzyme Conjugate-RTU to each well using a repeater pipette.
10. Incubate the plate, shaking at a fast speed (**600-800 rpm**) on an orbital microplate shaker, for **30 minutes** at room temperature.
11. Aspirate and wash each strip **5 times** with the Wash Solution using an automatic microplate washer.
12. Add **100 µL** of the TMB chromogen solution to each well using a precision pipette. Avoid exposure to direct sunlight.
13. Incubate the wells, shaking at **600-800 rpm** on an orbital microplate shaker, for **10-12 minutes** at room temperature.
NOTE: Visually monitor the color development to optimize the incubation time.
14. Add **100 µL** of the stopping solution to each well using a precision pipette. Read the absorbance of the solution in the wells **within 10 minutes**, using a microplate reader set to **450 nm**.
NOTE: Zero calibrator (Cal. A) should be programmed as "Blank" while reading the optical density. If instrument has a wavelength correction, set the instrument to dual wavelength measurement at 450 nm with background wavelength correction at 630 nm.

RESULTS

NOTE: The results in this package insert were calculated by plotting the data on a log vs. log scale and using a cubic regression curve-fit. Other data reduction methods may give slightly different results.

1. Calculate the mean optical density (OD) for each calibrator, Control, or Unknown.
2. Plot the log of the mean OD readings for each of the Calibrators along the y-axis versus log of the AMH concentrations in ng/mL along the x-axis, using a cubic regression curve-fit.
3. Determine the AMH concentrations of the unknowns from the calibration curve by matching their mean OD readings with the corresponding AMH concentrations.
4. Any sample reading higher than the highest Calibrator should be appropriately diluted with the 0 ng/mL (Cal A / Sample Diluent) and re-assayed.

5. Any sample reading lower than the analytical sensitivity should be reported as such.
6. Multiply the value by a dilution factor, if required.

LIMITATIONS

The reagents supplied in this kit are optimized to measure AMH levels in Porcine serum. If there is evidence of microbial contamination or excessive turbidity in a reagent, discard the vial. For assays employing antibodies, the possibility exists for interference by heterophile antibodies in the samples⁴.

QUALITY CONTROL

- Each laboratory should establish mean values and acceptable ranges to assure proper performance.
- Each laboratory should establish internal AMH controls ranges. The results should fall within established confidence limits.
- A full calibration curve, and control, should be included in each assay.
- TMB should be colorless. Development of any color may indicate reagent contamination or instability.

REPRESENTATIVE CALIBRATION CURVE DATA

Well Number	Well Contents Calibrators	Mean Absorbance	Conc (ng/mL)
A1, A2	A	0.032 (Blank)	0
B1, B2	B/2	0.058	0.125
C1, C2	B	0.111	0.25
D1, D2	C	0.225	0.5
E1, E2	D	0.449	1.0
F1, F2	E	0.847	2.0
G1, G2	F	1.651	4.0
H1, H2	G	2.936	8.0

CAUTION: The above data must not be employed in lieu of data obtained by the user in the laboratory

ANALYTICAL CHARACTERISTICS

All analytical characteristics are stated in ng/mL (1 ng/mL AMH = 7.14 pM)

Analytical Sensitivity:

The analytical sensitivity in the Porcine AMH ELISA assay, as calculated by the interpolation of mean plus two standard deviations of 16 replicates of calibrator A (0 ng/mL) and calibrator B (0.28 ng/mL), is **0.055 ng/mL**.

Linearity:

Multiple dilutions of the two porcine samples containing various AMH levels were diluted with Calibrator A/sample diluent. The % recovery on individual samples is represented in the following table.

Sample	Dilution Factor	Expected Conc. (ng/mL)	Observed Conc. (ng/mL)	% Recovery
1	Neat	2.809	NA	NA
	1:2	1.405	1.411	100%
	1:4	0.702	0.698	99%
	1:8	0.351	0.368	105%
	1:16	0.176	0.176	100%
2	Neat	3.122	NA	NA
	1:2	1.561	1.673	107%
	1:4	0.781	0.844	108%
	1:8	0.390	0.439	112%

Imprecision:

Reproducibility of the Porcine AMH ELISA assay was determined in a study using four samples over 12 runs. The study included two controls (n=48) and two samples (n=40, n=48 respectively). Representative data were calculated and are presented in the following table.

Sample	Mean (ng/mL)	Within run		Between run		Total	
		SD	CV	SD	CV	SD	CV
CI	0.8	0.04	4.9%	0.03	4.2%	0.05	6.4%
CII	2.4	0.07	2.8%	0.07	2.9%	0.1	4.0%
S-1	3.2	0.08	2.7%	0.06	1.9%	0.1	3.3%
S-2	8.2	0.43	5.2%	0.00	0.0%	0.43	5.2%

REFERENCES

1. HHS Publication, 6th ed., 2020. Biosafety in Microbiological and Biomedical Laboratories. Available https://www.cdc.gov/labs/pdf/SF_19_308133-A_BMBL6_00-BOOK-WEB-final-3.pdf
2. DHHS (NIOSH) Publication No. 78-127, August 1976. Current Intelligence Bulletin 13 - Explosive Azide Hazard. Available <http://www.cdc.gov/niosh>.
3. Approved Guideline – Procedures for the Handling and Processing of Blood Specimens, H18-A3. 2004. Clinical and Laboratory Standards Institute.
4. Kricka L. Interferences in immunoassays – still a threat. Clin Chem 2000; 46: 1037-1038.

This assay is intended for Research Use Only.

The Ansh Labs logo is a trademark of Ansh Labs.



Manufactured by:
Ansh Labs
445 Medical Center Blvd.
Webster, TX 77598-4217, U.S.A.

For Illustrative Purposes Only
Refer to package insert included with
the product for exact specifications.